

Reagecon

A CALIBRE SCIENTIFIC COMPANY



ISO 17034 Certified Reference Materials

Conductivity Standards, pH Buffer Standards and Sucrose in Water (Brix) Standards

> **Apex Chemicals Co.,Ltd.**

Head Office : 2034/87, Italthai Tower 19th Floor, New Petchburi Road, Bangkok, Huaykwang, Bangkok, Thailand 10310

T. 02-038-9999

@Apexchemicals

info@apexchemicals.co.th

Apexchemicals Co.,Ltd.

www.apexchemicals.co.th



About Reagecon

Reagecon, part of the Calibre Scientific Group of companies is one of the largest producers of Physical and Chemical Standards. The company is based in an 8,000 sq. metre facility that includes a large suite of manufacturing, Quality Control and Research and Development laboratories in Shannon, Ireland with sales offices in Shanghai and North America, Europe and the UK through our Calibre Scientific sister companies. Reagecon employs 100 people, 50% are chemistry or science graduates and most are involved in the Development, Production, Testing, Quality Control and Sales & Marketing of over 6,000 product references that we currently produce. We have a very active R&D programme and develop and bring to market many hundreds of new standards, every year.

All Reagecon manufactured products are underpinned by and demonstrate our position as a centre of excellence in the science of Metrology. Product is manufactured, tested, and certified under the applicable ISO/IEC 17025 (A2LA Ref: 6739.03) or ISO/IEC 17034 (A2LA Ref: 6739.01) accreditation or ISO/IEC 17025 (A2LA Ref: 6739.02) for Calibration, in one of our 20 specially equipped laboratories.

The resulting product is classified within one of 54 product families, these families are then grouped and promoted under 7 main product headings, as listed below:-


- ✓ Electrochemistry Standards
- ✓ Cation and Anion Standards
- ✓ Pharmacopoeia Reagents and Standards
- ✓ Physicochemical Standards
- ✓ Total Organic and Inorganic Carbon Standards
- ✓ Volumetric Solutions for Titration
- ✓ Customised Standards and Reagents



The Reagecon Hierarchy of Standards

Traditionally, Reagecon's manufactured products were on the lower end of the value chain and fitted into the classification of working and secondary standards. The development and production of such standards was consistent with our main technical competence (method validation/accreditation).

Standards Value Chain

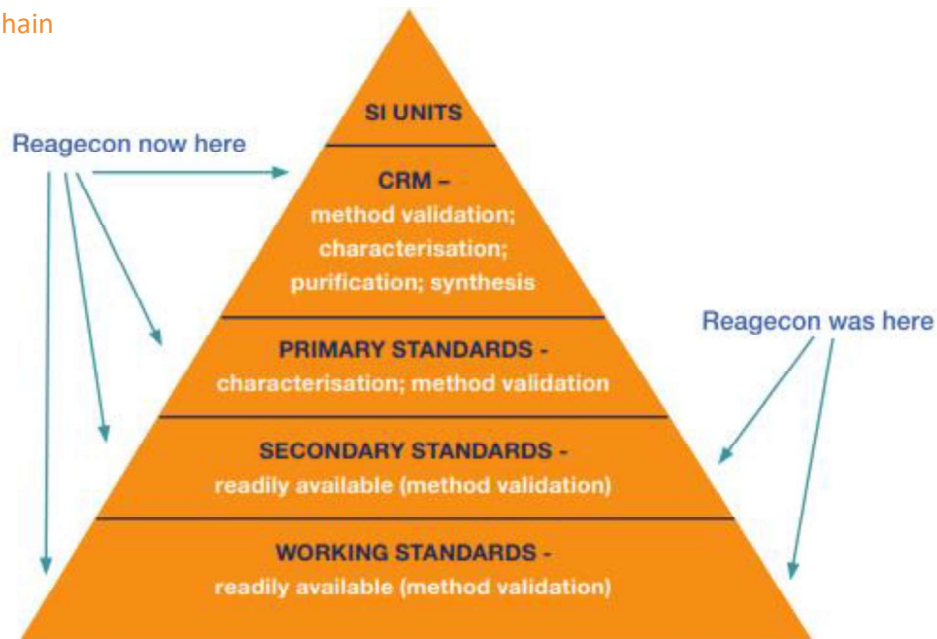

In recent years, we have escalated dramatically the range of working and secondary standards that we offer. Because of our recently developed ability to perform raw material characterisation we are now also producing Primary Standards and Certified Reference Materials. In the past the production of standards at the higher end of the value chain such as Primary Standards and Certified Reference Materials was the preserve of government funded agencies such as the National Institute of Science and Technology (NIST) in Washington, DC. Now, due to affordable technology, a number of privately funded companies have developed and are marketing primary standards and Certified Reference Materials. These companies generally have well-developed characterisation, purification and synthesis capability. Reagecon has grasped these opportunities with enthusiasm and are a leading producer of such materials.

As a producer of Metrological Standards we are concerned with enabling the end user (analyst) to achieve an analytical result that is fit for purpose and to provide proof of the correctness of that result. These two objectives are achieved through the following:

- ✓ Accreditation
- ✓ Traceability
- ✓ Accuracy
- ✓ Precision
- ✓ Sensitivity
- ✓ Limit of Detection (LOD)
- ✓ Reproducibility
- ✓ Measurement Uncertainty
- ✓ Comparability

Calibration Standards are critical to ensuring that an analysts sample measurements have the accuracy, traceability and comparability required so that actions taken based upon these sample measurements have validity. Reagecon's metrological expertise enables us to consistently produce Certified Reference Materials and Calibration Standards that gives their users confidence in the generated sample measurements.

Conductivity Standards

ISO 17034 Certified Reference Materials



Reagecon manufacture a range of Conductivity Certified Reference Materials (CRMs), which are manufactured and certified in accordance with the requirements of ISO 17034.

Our ISO 17034 Conductivity CRM range covers 20 $\mu\text{S}/\text{cm}$ to 10,000 $\mu\text{S}/\text{cm}$ and are accurate to a specification of $\pm 1\%$.

All are manufactured to exacting specifications with an extended shelf life and stability, even after opening the bottle.

Reagecon is the largest producer of Conductivity Standards and is credited with the invention of low level aqueous standards. The company is still the only producer worldwide with the capability to manufacture and stabilise these products at such low levels (1.3 $\mu\text{S}/\text{cm}$) of conductivity.

Summary of Features & Benefits

- ✓ Manufactured and certified in accordance with the requirements of ISO 17034
- ✓ All directly traceable to NIST standard reference materials. These products meet the specification requirements of all the major Pharmacopoeias
- ✓ Accurate to $\pm 1\%$ $\mu\text{S}/\text{cm}$ of target value
- ✓ Manufactured to exacting specifications with an extended shelf life and stability, even after opening the bottle.
- ✓ No shipping, storage or disposal issues
- ✓ Consistency of product – Independent, Traceable, Certified
- ✓ Certification Reports and Safety Data Sheets available online

Non-Hazardous

As Reagecon's Conductivity Standards are aqueous, they are non-hazardous. They offer the following benefits over solvent-based Conductivity Standards

- ✓ Ease and cost of shipping, without the need to provide hazardous goods' paperwork
- ✓ Reduced Health & Safety requirements for storage and use
- ✓ Ease and cost of disposal - solvent-based Conductivity Standards require expensive, specialised disposal to comply with environmental regulations.

Stability

As a result of the extensive R&D that led to our innovative manufacturing process, Reagecon can guarantee the stability of their complete range of Conductivity Standards over their entire shelf life. The stability offered by Reagecon's Conductivity Standards varies from that of their competitors in one vital area. We can guarantee that our Conductivity Standards will remain within specification (up to their expiry date) right through their working life, regardless of when the bottle was first opened provided Good Laboratory Practice is adhered to. This eliminates the need to open a fresh bottle of Standard every time the product is used. The shelf life of our Conductivity CRMs from their date of manufacture are given below.

| Conductivity Value ($\mu\text{S}/\text{cm}$) | Shelf Life |
|--|------------|
| 20 – 147 | 12 months |
| 200 – 10,000 | 18 months |

Matrix Matched

The matrix of a solution is defined as "the components of the sample other than the analyte". In all analytical measurements, it is of utmost importance that the matrix of the Standard and the sample are the same. As conductivity measurement is, in the main, a water quality measurement, the Standard used should also have an aqueous matrix. Reagecon's Conductivity Standards are all aqueous based, thereby eliminating any errors attributable to matrix mismatch.

Accuracy

All Standards have a specification of $\pm 1\%$ this high level of accuracy enables the Standards to be used as calibrators and/or controls in fulfilment of the most exacting industrial statutory requirements, for example the United States Pharmacopoeia monograph for Water for Injection.

Conductivity Standards

ISO 17034 Certified Reference Materials

Accreditation

Reagecon's conductivity measurement is covered in the scope of our accreditation to ISO 17025 "General Requirements for the competence of Calibration and Testing Laboratories" and its predecessor, EN 45001, since 1990. Reagecon is now delighted to also offer Conductivity Certified Reference Materials which are compliant to the requirements of ISO 17034. Achieving accreditation involves fulfilling many highly technical criteria, including fully validating our test methods and instrumentation systems and characterising our measurement uncertainty. Reagecon's accreditation proves the technical competence of our personnel, the technical validity of our test procedures and the traceability of our measurements. Therefore, in purchasing a Conductivity Standard from us, not only do you have transparent traceability to primary standards, but you also have confidence that our standards are of a well-defined and tightly controlled specification.

All values are Certified & Traceable

Comprehensive Certification Reports are available for all of Reagecon's Conductivity Standards, including detailed information on:

- ✔ Product Number
- ✔ Lot Number
- ✔ Expiry Date
- ✔ Mean Specific Conductance
- ✔ Date of Measurement
- ✔ Assay Limits
- ✔ Test Method Used
- ✔ Uncertainty of Measurement and Traceability Data

The complete range is traceable to primary standards from the United States National Institute for Standards and Technology (NIST). The traceability of these Standards is proven by the inclusion of conductivity testing in our ISO 17025 and ISO 17034 accreditation. It is a fundamental requirement of ISO 17025 and ISO 17034 that traceability is proven.

Temperature Coefficient of Variation

Reagecon's Standards are aqueous based and consequently have a very low temperature coefficient of variation. Non-aqueous Standards have a very high coefficient of variation which leads to measurement error and renders the products totally unsuitable for non-temperature controlled conditions, or field work.

Conductivity Standards at 25°C

ISO 17034 Certified Reference Materials (CRMs)

| Item No. | Description | UoM |
|-------------|---|-------|
| CRMCSKC20 | Conductivity Standard 20 $\mu\text{S}/\text{cm} \pm 1\%$ at 25°C | 500ml |
| CRMCSKC50 | Conductivity Standard 50 $\mu\text{S}/\text{cm} \pm 1\%$ at 25°C | 500ml |
| CRMCSKC84 | Conductivity Standard 84 $\mu\text{S}/\text{cm} \pm 1\%$ at 25°C | 500ml |
| CRMCSKC100 | Conductivity Standard 100 $\mu\text{S}/\text{cm} \pm 1\%$ at 25°C | 500ml |
| CRMCSKCS | Conductivity Standard 147 $\mu\text{S}/\text{cm} \pm 1\%$ at 25°C | 500ml |
| CRMCSKC200 | Conductivity Standard 200 $\mu\text{S}/\text{cm} \pm 1\%$ at 25°C | 500ml |
| CRMCSKC500 | Conductivity Standard 500 $\mu\text{S}/\text{cm} \pm 1\%$ at 25°C | 500ml |
| CRMCSKC1000 | Conductivity Standard 1000 $\mu\text{S}/\text{cm} \pm 1\%$ at 25°C | 500ml |
| CRMCSKCL | Conductivity Standard 1413 $\mu\text{S}/\text{cm} \pm 1\%$ at 25°C | 500ml |
| CRMCSKC2M | Conductivity Standard 2000 $\mu\text{S}/\text{cm} \pm 1\%$ at 25°C | 500ml |
| CRMCSKC3M | Conductivity Standard 3000 $\mu\text{S}/\text{cm} \pm 1\%$ at 25°C | 500ml |
| CRMCSKC5M | Conductivity Standard 5000 $\mu\text{S}/\text{cm} \pm 1\%$ at 25°C | 500ml |
| CRMCSKC10M | Conductivity Standard 10,000 $\mu\text{S}/\text{cm} \pm 1\%$ at 25°C | 500ml |

Extensive Range of Values

Together with our Conductivity CRM range Reagecon also offer over 45 different values of Conductivity Standards ranging from as low as 1.3 $\mu\text{S}/\text{cm}$ to as high as 500,000 $\mu\text{S}/\text{cm}$ manufactured and tested in accordance with ISO 17025.

Unparalleled Technical Support

We have been manufacturing Conductivity Standards for over 30 years. In that time, we have built up a vast resource of technical expertise on all aspects of conductivity measurement. The members of Reagecon's Technical Services Department have written a comprehensive series of papers covering all the practical requirements for accurate conductivity measurement. These papers are available via our website www.reagecon.com

pH Buffer Standards

ISO 17034 Certified Reference Materials



Reagecon produce a range of pH Buffer Certified Reference Materials (CRMs), which are manufactured and certified in accordance with the requirements of ISO 17034.

Our ISO 17034 pH Buffer CRMs range covers pH 1.697 to pH 12.00 inclusive.

All are manufactured to exacting specifications with an extended shelf life and stability, even after opening the bottle.

Traceability

These pH buffer CRMs are directly traceable to the IUPAC pH scale by an unbroken chain of traceability. Reagecon achieve this traceability through a series of comparisons, with the key reference materials being Standard Reference Materials (SRMs) manufactured by NIST.

For proof of traceability, all these comparisons must be made in a technically valid manner and the accuracy of each step must be quantified by calculating the associated Uncertainty of Measurement. Reagecon's pH Buffer Standards meet the ISO definition of traceability: "The ability to relate measurements back to a stated reference (usually an international standard) through an unbroken chain of comparisons, each having stated uncertainties of measurement." Reagecon's traceability claims are guaranteed by our accreditation to ISO 17034 and ISO 17025.

pH Buffer CRMs are supplied with a detailed Certification Report which outlines traceability to NIST.

Why use traceable pH Buffers ?

Your pH measurements can only be as good as the pH Buffers that you use. If your pH calibration is made using traceable pH Buffers then you have a direct link to the International pH scale for your measurements. Without this link, you are not entitled to report your measurements in pH units so the number displayed on your pH meter is just that - a number and is not a pH value. The common link that is achieved by traceability allows comparability of results regardless of:

- ✓ When the measurements were made
- ✓ Where the measurements were made
- ✓ What instrumentation was used to make the measurements

Traceable analysis is necessary for consistency and universal acceptance of your pH results - including acceptance by regulatory bodies.

Control Buffers

For increased confidence in their test measurements analysts should regularly measure the pH of a Control Standard. If an acceptable value is obtained from the Control Standard measurement then the analysts, can have improved confidence that their test measurements will be correct.

Summary of Features & Benefits

- ✓ Manufactured and certified in accordance with the requirements of ISO 17034
- ✓ NIST traceable
- ✓ Directly traceable to the IUPAC pH scale by an unbroken chain of traceability. Reagecon achieve this traceability through a series of comparisons, with the key reference materials being Standard Reference Materials (SRMs) manufactured by NIST
- ✓ Values specified at specific temperature e.g. 20°C/25°C
- ✓ Manufactured to exacting specifications with an extended shelf life & stability
- ✓ Lot numbers and expiry dates are available via the product label for user convenience
- ✓ Consistency of product – Independent, Traceable, Certified
- ✓ Certification Report and Safety Data Sheets available online

pH Buffer Standards

ISO 17034 Certified Reference Materials

Fully Accredited

Reagecon's pH analysis is accredited to ISO 17034 and ISO 17025 "General requirements for the competence of testing and calibration laboratories". Reagecon's accreditation to ISO 17034 and ISO 17025 gives independent proof of three key areas:

- Our pH analysis is technically valid and is carried out in a thoroughly controlled manner by highly - qualified staff
- Our claims over the accuracy of our pH analysis are valid and we have properly quantified our accuracy in our uncertainty of measurement calculations
- Our pH analysis is traceable to NIST SRMs

Why take chances with your pH buffer supplier's traceability? By using buffers from a manufacturer that holds ISO 17034 and ISO 17025 accreditation you have a guarantee of traceability.

Stability

Reagecon's pH Buffers have been specially formulated to ensure their stability. The packaging bottles that we use have also been selected and tested to provide maximum stability. We have conducted stability trials on both freshly-opened and part-full bottles of our pH Buffers to validate their shelf-life - an example is given in Figure 2.

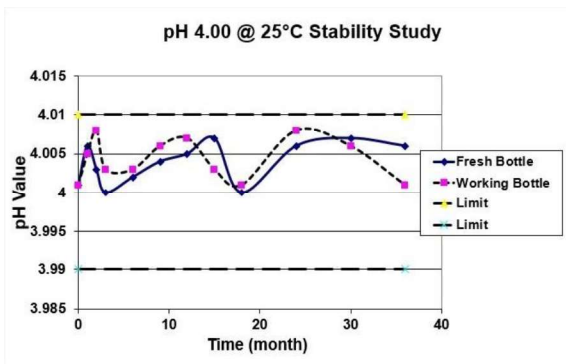


Figure 2: Stability Data for Reagecon pH 4.00 @ 25 °C

pH Buffer Standards at 20°C NIST Values ISO 17034 Certified Reference Materials (CRMs)

| Item No. | Description | UoM |
|-----------|--|-------|
| CRM103788 | Buffer Standard pH 3.788 ± 0.010 at 20°C NIST Value | 500ml |
| CRM104001 | Buffer Standard pH 4.001 ± 0.010 at 20°C NIST Value | 500ml |
| CRM106881 | Buffer Standard pH 6.881 ± 0.010 at 20°C NIST Value | 500ml |
| CRM107429 | Buffer Standard pH 7.429 ± 0.010 at 20°C NIST Value | 500ml |
| CRM109225 | Buffer Standard pH 9.225 ± 0.010 at 20°C NIST Value | 500ml |
| CRM110062 | Buffer Standard pH 10.062 ± 0.010 at 20°C NIST Value | 500ml |

pH Buffer Standards at 25°C DIN 19266 ISO 17034 Certified Reference Materials (CRMs)

| Item No. | Description | UoM |
|-----------|---|-------|
| CRM101679 | Buffer Standard pH 1.679 ± 0.010 at 25°C DIN 19266 | 500ml |
| CRM103776 | Buffer Standard pH 3.776 ± 0.010 at 25°C DIN 19266 | 500ml |
| CRM104005 | Buffer Standard pH 4.005 ± 0.010 at 25°C DIN 19266 | 500ml |
| CRM10687 | Buffer Standard pH 6.865 ± 0.010 at 25°C DIN 19266 | 500ml |
| CRM107413 | Buffer Standard pH 7.413 ± 0.010 at 25°C DIN 19266 | 500ml |
| CRM109180 | Buffer Standard pH 9.180 ± 0.010 at 25°C DIN 19266 | 500ml |
| CRM110012 | Buffer Standard pH 10.012 ± 0.010 at 25°C DIN 19266 | 500ml |

pH Buffer Standards at 25°C DIN 19267 ISO 17034 Certified Reference Materials (CRMs)

| Item No. | Description | UoM |
|-----------|--|-------|
| CRM103065 | Buffer Standard pH 3.06 ± 0.02 at 25°C DIN 19267 | 500ml |
| CRM104655 | Buffer Standard pH 4.65 ± 0.01 at 25°C DIN 19267 | 500ml |
| CRM106795 | Buffer Standard pH 6.79 ± 0.01 at 25°C DIN 19267 | 500ml |
| CRM109235 | Buffer Standard pH 9.23 ± 0.01 at 25°C DIN 19267 | 500ml |

pH Buffer Standards

ISO 17034 Certified Reference Materials

pH Buffer Standards at 20°C ISO 17034 Certified Reference Materials (CRMs)

| Item No. | Description | UoM |
|----------|---|-----|
| CRM1020 | Buffer Standard pH 2.00 ± 0.02 at 20°C | 1L |
| CRM1030 | Buffer Standard pH 3.00 ± 0.02 at 20°C | 1L |
| CRM1040 | Buffer Standard pH 4.00 ± 0.01 at 20°C | 1L |
| CRM1050 | Buffer Standard pH 5.00 ± 0.01 at 20°C | 1L |
| CRM1060 | Buffer Standard pH 6.00 ± 0.01 at 20°C | 1L |
| CRM1070 | Buffer Standard pH 7.00 ± 0.01 at 20°C | 1L |
| CRM1080 | Buffer Standard pH 8.00 ± 0.01 at 20°C | 1L |
| CRM1090 | Buffer Standard pH 9.00 ± 0.01 at 20°C | 1L |
| CRM1100 | Buffer Standard pH 10.00 ± 0.01 at 20°C | 1L |
| CRM1110 | Buffer Standard pH 11.00 ± 0.05 at 20°C | 1L |
| CRM1120 | Buffer Standard pH 12.00 ± 0.05 at 20°C | 1L |

| Item No. | Description | UoM |
|-----------|--|-------|
| CRM10685 | Buffer Standard pH 6.80 ± 0.01 at 20°C | 500ml |
| CRM10925 | Buffer Standard pH 9.20 ± 0.01 at 20°C | 500ml |
| CRM109220 | Buffer Standard pH 9.22 ± 0.01 at 20°C | 500ml |

pH Buffer Standards at 25°C ISO 17034 Certified Reference Materials (CRMs)

| Item No. | Description | UoM |
|-----------|---|-----|
| CRM102025 | Buffer Standard pH 2.00 ± 0.02 at 25°C | 1L |
| CRM103025 | Buffer Standard pH 3.00 ± 0.02 at 25°C | 1L |
| CRM104025 | Buffer Standard pH 4.00 ± 0.01 at 25°C | 1L |
| CRM105025 | Buffer Standard pH 5.00 ± 0.01 at 25°C | 1L |
| CRM106025 | Buffer Standard pH 6.00 ± 0.01 at 25°C | 1L |
| CRM107025 | Buffer Standard pH 7.00 ± 0.01 at 25°C | 1L |
| CRM108025 | Buffer Standard pH 8.00 ± 0.01 at 25°C | 1L |
| CRM109025 | Buffer Standard pH 9.00 ± 0.01 at 25°C | 1L |
| CRM110025 | Buffer Standard pH 10.00 ± 0.01 at 25°C | 1L |
| CRM111025 | Buffer Standard pH 11.00 ± 0.05 at 25°C | 1L |
| CRM112025 | Buffer Standard pH 12.00 ± 0.05 at 25°C | 1L |

| Item No. | Description | UoM |
|-------------|---|-------|
| CRM1068525 | Buffer Standard pH 6.80 ± 0.01 at 25°C | 500ml |
| CRM1068805 | Buffer Standard pH 6.86 ± 0.01 at 25°C | 500ml |
| CRM1094025 | Buffer Standard pH 9.40 ± 0.01 at 25°C | 500ml |
| CRM11001525 | Buffer Standard pH 10.01 ± 0.01 at 25°C | 500ml |

pH Buffer Standards at 20°C Colour Coded ISO 17034 Certified Reference Materials (CRMs)

| Item No. | Description | UoM |
|-----------|---|-------|
| CRM10405C | Buffer Standard pH 4.00 ± 0.01 at 20°C Colour Coded (Red) | 500ml |
| CRM10705C | Buffer Standard pH 7.00 ± 0.01 at 20°C Colour Coded (Yellow) | 500ml |
| CRM11005C | Buffer Standard pH 10.00 ± 0.01 at 20°C Colour Coded (Blue) | 500ml |

pH Buffer Standards at 25°C Colour Coded ISO 17034 Certified Reference Materials (CRMs)

| Item No. | Description | UoM |
|-------------|---|-------|
| CRM1040525C | Buffer Standard pH 4.00 ± 0.01 at 25°C Colour Coded (Red) | 500ml |
| CRM1070525C | Buffer Standard pH 7.00 ± 0.01 at 25°C Colour Coded (Yellow) | 500ml |
| CRM1100525C | Buffer Standard pH 10.00 ± 0.01 at 25°C Colour Coded (Blue) | 500ml |

pH Buffer Standards at 20°C High Resolution Colour Coded ISO 17034 Certified Reference Materials (CRMs)

| Item No. | Description | UoM |
|------------|---|-------|
| CRM104000C | Buffer Standard pH 4.000 ± 0.010 at 20°C High Resolution Colour Coded (Red) | 500ml |
| CRM107000C | Buffer Standard pH 7.000 ± 0.010 at 20°C High Resolution Colour Coded (Yellow) | 500ml |
| CRM110000C | Buffer Standard pH 10.000 ± 0.010 at 20°C High Resolution Colour Coded (Blue) | 500ml |

pH Buffer Standards at 25°C High Resolution Colour Coded ISO 17034 Certified Reference Materials (CRMs)

| Item No. | Description | UoM |
|-------------|---|-------|
| CRMH40525C | Buffer Standard pH 4.000 ± 0.010 at 25°C High Resolution Colour Coded (Red) | 500ml |
| CRMH70525C | Buffer Standard pH 7.000 ± 0.010 at 25°C High Resolution Colour Coded (Yellow) | 500ml |
| CRMH100525C | Buffer Standard pH 10.000 ± 0.010 at 25°C High Resolution Colour Coded (Blue) | 500ml |

pH Buffer Standards at 25°C Technical Colour Coded ISO 17034 Certified Reference Materials (CRMs)

| Item No. | Description | UoM |
|----------|---|-------|
| CRMTB401 | Buffer Standard pH 4.01 ± 0.02 at 25°C Technical Colour Coded (Red) | 500ml |
| CRMTB460 | Buffer Standard pH 4.60 ± 0.02 at 25°C Technical Colour Coded (Red) | 500ml |
| CRMTB700 | Buffer Standard pH 7.00 ± 0.02 at 25°C Technical Colour Coded (Yellow) | 500ml |
| CRMTB921 | Buffer Standard pH 9.21 ± 0.02 at 25°C Technical Colour Coded (Blue) | 500ml |
| CRMTB100 | Buffer Standard pH 10.00 ± 0.02 at 25°C Technical Colour Coded (Blue) | 500ml |

Sucrose in Water (Brix) Standards

ISO 17034 Certified Reference Materials

Reagecon manufacture a range of Sucrose in Water (Brix) Certified Reference Materials (CRMs), which are manufactured and certified in accordance with the requirements of ISO 17034 and ISO 17025. Product measurement uncertainty is computed on a batch to batch basis, guaranteed to never exceed ± 0.15 °Brix.



These products are used primarily either as a calibrant or analytical control solution in Refractive Index based methods of Brix value determinations, they can also be used to validate appropriate test methods or qualify a refractometer for use in a regulated industry.

Our Sucrose in Water Standards have a shelf life of 20 weeks and are produced in accordance with ICUMSA guidelines.

Sucrose in Water (Brix) ISO 17034 Certified Reference Materials (CRMs)

| Item No. | Description | UoM |
|----------|-------------------------------|------|
| BS05 | 5% Sucrose in Water (Brix) | 15ml |
| BS07 | 7% Sucrose in Water (Brix) | 15ml |
| BS10 | 10% Sucrose in Water (Brix) | 15ml |
| BS112 | 11.2% Sucrose in Water (Brix) | 15ml |
| BS115 | 11.5% Sucrose in Water (Brix) | 15ml |
| BS12 | 12% Sucrose in Water (Brix) | 15ml |
| BS125 | 12.5% Sucrose in Water (Brix) | 15ml |
| BS15 | 15% Sucrose in Water (Brix) | 15ml |
| BS20 | 20% Sucrose in Water (Brix) | 15ml |
| BS25 | 25% Sucrose in Water (Brix) | 15ml |
| BS30 | 30% Sucrose in Water (Brix) | 15ml |
| BS35 | 35% Sucrose in Water (Brix) | 15ml |
| BS40 | 40% Sucrose in Water (Brix) | 15ml |
| BS45 | 45% Sucrose in Water (Brix) | 15ml |
| BS50 | 50% Sucrose in Water (Brix) | 15ml |
| BS55 | 55% Sucrose in Water (Brix) | 15ml |
| BS60 | 60% Sucrose in Water (Brix) | 15ml |

Summary of Features & Benefits

- ✔ Extended shelf life - 20 weeks (Manufactured in accordance with ICUMSA guidelines)
- ✔ Manufactured and certified in accordance with the requirements of ISO 17034 and ISO 17025
- ✔ Can be used with any brand of refractometer
- ✔ Extensive range (1-60% mass/mass Sucrose in Water Solutions)
- ✔ Product measurement uncertainty is computed on a batch to batch basis, guaranteed to never exceed ± 0.15 °Brix
- ✔ Presented in a convenient high quality dropper bottle
- ✔ Ready to Use
- ✔ Consistency of product – Independent, Traceable, Certified
- ✔ Certification Reports and Safety Data Sheets available online



Reagecon

A CALIBRE SCIENTIFIC COMPANY

For further information or enquiries, please contact us:

Tel: +353 61 472622

Email: sales@reagecon.ie

www.reagecon.com